

# Construction of an Ultra Low Temperature STM with a Bottom Loading Mechanism

T. Matsui<sup>a</sup>, H. Kambara<sup>a</sup>, I. Ueda<sup>a</sup>, T. Shishido<sup>a</sup>, and Hiroshi Fukuyama<sup>a,1</sup>

<sup>a</sup>Department of Physics, University of Tokyo, 7-3-1 Hongo Bunkyo-ku, Tokyo 113-0033, Japan

---

## Abstract

We have constructed and tested an ultra-low temperature scanning tunneling microscope that works with an atomic resolution at ultra low temperatures ( $T \geq 160$  mK) in magnetic fields ( $B \leq 6$  T) in ultra high vacuum (UHV). Clean sample surfaces can be prepared by several different methods and characterized by low energy electron diffraction (LEED) *in situ* of UHV. A unique bottom loading mechanism enables us to cool back to the base temperature within 3 hours after changing the sample and STM tip.

*Key words:* low temperature STM

---

## 1. Introduction

The scanning tunneling microscopy and spectroscopy (STM/STS) technique has recently become a powerful tool for low temperature experiments. This is because, with this technique, we can study a variety of low temperature phenomena ranging from adsorbed two dimensional solids to low  $T_c$  superconductors with extraordinary spatial resolutions.

Here we report the construction and test results of the first STM designed to work with an atomic resolution at ultra low temperatures (ULT) below 200 mK in magnetic fields up to 6 T. It has also capabilities of sample preparation and characterization *in situ* of UHV. After transferring the sample and tip to the STM head, it takes only 3 h to cool back to the base temperature. All these features make this new ULT-STM more versatile than previously constructed ones [1][2][3].

## 2. Designing

Since the designing of our ULT-STM has been already reported elsewhere [4] rather in detail, we will describe here mainly what have been changed from the original design.

We have replaced the 38 cm long copper rod, which thermally and mechanically connects the STM head to the mixing chamber (MC) of dilution refrigerator (DR) (see Fig.2 of ref. [4]), with a more rigid copper cage with three support rods. It was necessary to do so in order to improve mechanical rigidity of the system. Otherwise, the lateral atomic resolution was not obtained. Note that we have no anti-vibration mechanism such as spring loading one at low temperatures.

The thermal link to cool the sample and tip below 200 mK is based on three sintered silver-powder heat exchangers ( $4 \text{ m}^2$  surface area) packed in an epoxy capsule which is filled with liquid  $^3\text{He}$  ( $0.5 \text{ cm}^3$ ). This configuration was adopted to keep better thermal contact and electrical isolation between the sample, tip and MC. Each heat exchanger is sintered to a silver wire (1 mm  $\phi$ ) and connected either to the MC, sample or tip. In order to improve the high temperature performance, a  $25 \mu\text{m}$  thick Mylar sheet was inserted between the

---

<sup>1</sup> E-mail:hiroshi@phys.s.u-tokyo.ac.jp

silver wire and MC. The sample temperature is monitored with a RuO<sub>2</sub> resistance thermometer attached to the silver wire, which connects the sample to one of the heat exchangers.

The bottom loading mechanism for the sample and tip minimizes the access length from the UHV chamber to the STM head. We used a commercial DR [5] with a dewar which has demountable tails. The STM head [6] is made of silver based alloys which are non-magnetic and have small nuclear-spin heat capacities at ULT and high fields.

### 3. Test results

We have tested the cleavage mechanism, LEED characterization, precooling and sample/tip exchange mechanism using a Sr<sub>2</sub>RuO<sub>4</sub> single crystal. All these procedures have been done in UHV environment. Fig. 1(a) is a LEED pattern of the cleaved sample surface. It clearly shows the four-fold symmetry of SrO plane indicating successful cleavage [7]. The sample and tip were precooled by liquid nitrogen and helium flow down to 100 K and 7 K, respectively, within 40 min (see Fig. 2(a)). They were then transferred to the STM head (see the arrows v and vi in Fig. 2(b)). The STM head warmed up to 8 K temporarily by this transfer as well as by accompanying removal and installation of the 80 K and 4 K radiation baffles. However, in 20 min, it cooled down to 2 K due to a large heat capacity of <sup>3</sup>He-<sup>4</sup>He liquid mixture in the DR. During this exchange procedure, the <sup>3</sup>He circulation of DR was stopped, while the 1 K pot was kept running. It takes only 2 h for the MC to cool back to the base temperature (45 mK) after restarting the <sup>3</sup>He circulation.

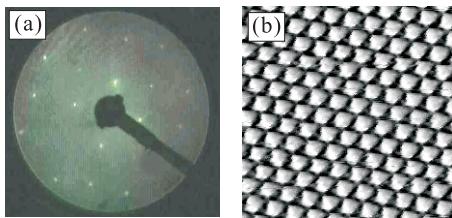


Fig. 1. (a) The LEED pattern measured at room temperature with an electron energy of 193 eV for a Sr<sub>2</sub>RuO<sub>4</sub> cleaved at 8 K. (b) The STM image of HOPG at 4.2 K (constant height mode;  $I = 0.4$  nA,  $V = 0.1$  V;  $2.5 \times 2.5$  nm<sup>2</sup>, PtIr tip).

Fig. 1(b) shows an STM image of HOPG transferred to the STM head in the same manner as described above. This image was taken at 4.2 K. Essentially similar images were obtained at 160 mK, the lowest sample temperature achieved in the first cooling run. The measured temperature difference between the MC and

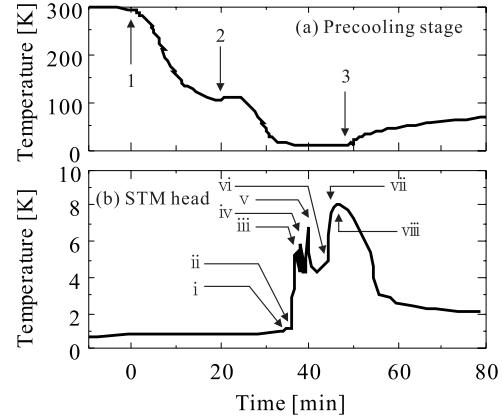


Fig. 2. (a) The time evolution of temperature of the precooling stage. The arrows indicate when we started precooling of the stage with liquid N<sub>2</sub> (1) and He flow (2) and when we stopped the He flow (3). (b) The time evolution of temperature of the STM head during sample/tip exchange. The arrows indicate when we removed 80 K (i) and 4 K radiation baffles (ii), sample (iii) and tip (iv), and when we installed new tip (v), new sample (vi) and the 4 K (vii) and the 80 K (viii) baffles.

sample indicates a large heat leak to the STM head of 20  $\mu$ W at most. We believe that a major source of the heat leak is radiation from the 4 K baffle whose temperature is probably much higher than 4 K because of insufficient radiation shielding at the dewar tail. This problem will be fixed in the next cooling run.

### Acknowledgements

We thank Yoshi Maeno for providing us a Sr<sub>2</sub>RuO<sub>4</sub> single crystal. This work was supported by Grants-in-Aid for Scientific Research from MEXT, Japan and ERATO project of JST.

### References

- [1] H. Fukuyama, H. Tan, T. Kumakura and M. Morishita, Czech. J. of Phys. **46**, (1996) Suppl. S5 2847.
- [2] S. H. Pan, E. W. Hudson and J. C. Davis, Rev. Sci. Instrum. **70**, (1999) 1459.
- [3] N. Moussy, H. Courtois and B. Pannetier, Rev. Sci. Instrum. **72**, (2001) 128.
- [4] T. Matsui, H. Kambara and H. Fukuyama, J. Low Temp. Phys. **121**, (2000) 803.
- [5] Oxford Instruments, model Kelvinox-100.
- [6] The STM head and UHV chamber were designed and developed as a collaboration with Unisoku Scientific Instruments.
- [7] H. Kambara, T. Matsui, K. Yokota, I. Ueda, T. Shishido, N. Kikugawa, Y. Maeno, H. Fukuyama, this conference.